

SHORT Implant Catalog

Since 1985 » Simple. Predictable. Profitable.







Continuing our efforts to simplify the surgical and restorative procedures, Bicon has created this condensed SHORT™ Implant catalog.

The items contained in this manual are those products which Bicon clinicians from around the world use 80% of the time. If a clinical situation arises in which other sizes of implants are required or if a different style of abutment is needed, please refer to Bicon's Complete Catalog or visit www.bicon.com to view our entire product line.



Bicon implants, abutments, instrumentation, and components are engineered, manufactured, packaged, and/or sterilized at ISO Certified facilities.

Bicon fulfills the stringent requirements of the European Directive 93/42/EEC for medical devices as well as strict adherence to the ISO 13485 standard.

THE BICON SYSTEM

A simple and elegant design that has remained unchanged and in continuous use since 1985.



BICON'S LOCKING TAPER

- ► Time-tested stable connection
- Proven bacterial seal


BICON'S SLOPING SHOULDER

- Space for bone over the implant
- Distributes occlusal stresses
- Preserves crestal bone

BICON'S PLATEAU DESIGN

- ► 30% more surface area
- No splinting necessary
- Callus bone formation
- Cortical-like Haversian bone between the fins

Diameter and Surface	Length	Well	Part Number		
4.5mm Integra-CP™ Implant	6.0mm	3.0mm	260-345-306		
4.5mm Integra-CP™ Implant	8.0mm	3.0mm	260-345-308	4.5 x 6	4.5 x 8
5.0mm Integra-CP™ Implant	5.0mm	3.0mm	260-350-305		
5.0mm Integra-CP™ Implant	6.0mm	3.0mm	260-350-306		
5.0mm Integra-CP™ Implant	8.0mm	3.0mm	260-350-308	5 x 5 5	x 6 5 x 8
6.0mm Integra-CP™ Implant	5.0mm	3.0mm	260-360-305		
6.0mm Integra-CP™ Implant	5.7mm	3.0mm	260-360-357	6 x 5	6 x 5.7



[‡]Available with a 2.0mm or a 2.5mm well. △Available with a 2.5mm or a 3.0mm well.

- Each implant is packaged with its appropriate healing plug.
- All implants are manufactured from Ti6Al4V.







^{*}Recommended for two stage surgical procedure.



Description Part Number

3.0mm Impression Post and Sleeve (2)

260-100-433

260-100-434

3.0mm Implant Level Impression Kit



3.0mm Impression Post Titanium



3.0mm Impression Sleeve Plastic



3.0mm Implant Analog Titanium

- The impression kit contains an impression post, sleeve, and implant analog.
- Narrower implant well diameters require a different impression post, sleeve, and implant analog.
- See Complete Catalog for other post diameters and sleeves.


Technique



1 Insert green impression post for 3.0mm well implants using finger pressure.



2 Insert red impression post for 2.0mm well implants using finger pressure.



3 Snap on impression sleeve.



4 Snap on impression sleeve.



5 Inject impression material.



6 Withdraw impression and sleeves.



7 Assemble titanium posts and analogs.



8 Insert assembly into impression.



9 Pour a stone model.



NON-SHOULDERED ABUTMENTS

Description	Diameter	Height	Angle	Post	Part Number		
4.0 x 6.5mm 0° Abutment	4.0mm	6.5mm	0°	3.0mm	260-340-001	B	B
4.0 x 6.5mm 15° Abutment	4.0mm	6.5mm	15°	3.0mm	260-340-015	O°	15°
5.0 x 6.5mm 0° Abutment	5.0mm	6.5mm	0°	3.0mm	260-350-001		A
5.0 x 6.5mm 15° Abutment	5.0mm	6.5mm	15°	3.0mm	260-350-015	O°	15°
6.5 x 5.0mm 0° Abutment	6.5mm	5.0mm	0°	3.0mm	260-365-050		A
6.5 x 6.5mm 15° Abutment	6.5mm	6.5mm	15°	3.0mm	260-365-015	0°	15°

■ For additional abutment sizes see page 15–16.


- The non-shouldered abutments are designed for PFM restorations and are useful for the IAC restorations.
- Non-shouldered abutments are fully "preppable" and may be modified intra-orally or extra-orally.
- Clinicians may make direct impressions of non-shouldered abutments or make indirect impressions with the use of an impression sleeve.
- See Complete Catalog for information on emergence cuffs, impression sleeves, and transfer dies that are available.



Description	Diameter	Height	Angle	Post	Part Number		
5.0 x 2.0mm 0° Stealth Abutment	5.0mm	2.0mm	0°	3.0mm	260-300-301	1	1
5.0 x 2.0mm 10° Stealth Abutment	5.0mm	2.0mm	10°	3.0mm	260-300-302	0°	10°
5.0 x 4.0mm 0° Stealth Abutment	5.0mm	4.0mm	0°	3.0mm	260-300-321		4
5.0 x 4.0mm 10° Stealth Abutment	5.0mm	4.0mm	10°	3.0mm	260-300-322	0°	10°
6.5 x 2.0mm 0° Stealth Abutment	6.5mm	2.0mm	0°	3.0mm	260-300-601	1	
6.5 x 4.0mm 0° Stealth Abutment	6.5mm	4.0mm	0°	3.0mm	260-300-621	0°	0°



*Impression and Temporization Sleeves are packaged with each abutment.



- For additional abutment sizes see page 17–18.
- Designed for PFM restorations, all ceramic restorations, and Cerec® crowns.
- Impression sleeves, aluminum oxide sleeves, and transfer dies are available.

Temporary Abutments

Description	Diameter	Height	Post	Style	Part Number		
4.0 x 4.5mm Temporary Abutment	4.0mm	4.5mm	3.0mm	Titanium	260-340-345	4.0 >	x 4.5
5.0 x 4.5mm Temporary Abutment	5.0mm	4.5mm	3.0mm	Titanium	260-350-345		V
5.0 x 6.5mm Temporary Abutment	5.0mm	6.5mm	3.0mm	Titanium	260-350-365	5.0 x 4.5	5.0 x 6.5

Healing Abutments

Description		Hainba	Doot	Angla	Chulo	Davit Namelson		
Description	Diameter	Height	Post	Angle	Style	Part Number		
5.0 x 5.0mm 0° Healing Abutment	5.0mm	5.0mm	3.0mm	0°	Plastic	260-350-500		
5.0 x 8.0mm 0° Healing Abutment	5.0mm	8.0mm	3.0mm	0°	Plastic	260-350-800	5.0 x 5.0 5.0 x 8	5.0 x 8.0
6.5 x 5.0mm 0° Healing Abutment	6.5mm	5.0mm	3.0mm	0°	Plastic	260-365-500	6.5	\$ 5.0




- Temporary and Healing abutments are designed to help form and maintain a gingival sulcus on a temporary basis.
- Temporary and Healing abutments are designed for single stage surgical procedures.



Description	Height	Angle	Post	Part Number		
2.0mm 0° Brevis Abutment	2.0mm	0°	3.0mm	260-300-434	å	3
2.0mm 15° Brevis Abutment	2.0mm	15°	3.0mm	260-300-435	0°	15°
4.0mm 0° Brevis Abutment	4.0mm	0°	3.0mm	260-300-436	â	3
4.0mm 15° Brevis Abutment	4.0mm	15°	3.0mm	260-300-437	0°	15°

^{*}Each abutment is packaged with a titanium housing and o-ring.

Restorative Con	nponents		
Description	Part Number		
Brevis Abutment Chairside Kit	260-100-212	Rubber O-Ring	Brevis Housing
Brevis Impression Kit without Housing	260-100-218	Impression Cap	Aluminum Transfer Die
BREVIS [™]	3.0mm	3.0mm	A A





[•] See Complete Catalog for additional abutment heights that are available.



BICON SURGICAL KIT

Description Part Number

Comprehensive Surgical Kit 260-101-098





Advanced and Introductory Surgical Kits also available.

REGENERATIVE PRODUCTS



SynthoGraft™

Description	Particle Size	Grams per Vial	Vials	Part Number	
SynthoGraft™ Pure Phase Beta-Tricalcium Phosphate	50-500μm Small	0.5g	5	260-400-150	
SynthoGraft™ Pure Phase Beta-Tricalcium Phosphate	500-1000µm Large	0.5g	5	260-400-500	Synthe State So Soor

■ SynthoGraft[™] is also available in 0.25g, 1.0g, and 2.0g vials.



Resorbable Collagen Membrane

Description	Size	Part Number	
Bicon Resorbable Collagen Membrane	15 x 20 x 0.3mm	260-509-600	

■ Membranes are also available in sizes of 20 x 30mm and 30 x 40mm.

Resorbable Collagen Plug

Description	Size	Part Number	
Resorbable Collagen Plug (10)	10 x 20mm	260-509-400	



TWO STAGE SURGICAL TECHNIQUE

Two Stage Surgery Implant Insertion Technique



Extraction Site Envelope Scalloped



For the best emergence, drill a 2.0mm pilot hole (with external irrigation) 2.0mm deeper than the chosen implant length when adequate bone height is available.



Use paralleling pins to facilitate alignment when placing multiple implants.



Place an abutment with a 2.0mm post into pilot hole and confirm appropriateness with a vacu-press template.



Widen socket with sequentially larger reamers **without irrigation** at a maximum of 50 RPM. In this case, a 5.0 x 6.0mm implant has been chosen so the final bur used also has a diameter of 5.0mm.



Place harvested autogenous bone, intermittently removed from the flutes of the reamer burs, into a silicone dappen dish for later use.




Harvest bone debris from reamer flutes and socket.



The implant's sterile blister pack is dropped onto a sterile tray prior to removing its Tyvek® backing before the implant's inner packaging is cut with a pair of scissors.



Remove implant from poly bag.



Seat implant by tapping gently on healing plug or directly into the implant well with an appropriate seating tip.



Cut healing plug. Ensure that no sharp edges remain that could irritate soft tissue.



Place harvested bone graft over shoulder of implant. See Step #6 above.



Close and wait a minimum of ten to twelve weeks for osseointegration.

TWO STAGE SURGICAL TECHNIQUE




Implant Uncovering Technique and Placement of Abutment



Expose the implant in aesthetic areas with a semilunar crestal incision.



Make split-thickness buccal flap.




Remove healing plug with a healing plug removal instrument.



Place appropriate guide pin to check integration and angulation.




Remove excess bone with sulcus reamer corresponding to the chosen abutment with either threaded knob or straight handle.



Flush and dry implant well with a cotton tip.



Insert chosen abutment.



Use a template to confirm appropriateness of abutment prior to engagement of locking taper connection, then tap on abutment in long axis of abutment post to engage locking taper.



Place an emergence cuff or temporization sleeve onto abutment and modify, if necessary.



Inject acrylic around emergence cuff or temporization sleeve and into the vacu-press template.



Place template to form temporary crown.



Remove and polish acrylic confluent with emergence cuff or temporization sleeve to help form the gingival sulcus.




Wait for soft tissue healing prior to taking final impression.



NON-SHOULDERED ABUTMENT RESTORATIONS


Porcelain Fused to Metal and Integrated Abutment Crown™







Porcelain Fused to Metal and All-Ceramic





TEMPORIZATION OPTIONS

OPTION ONE: TRANSITIONAL RESTORATION WITH SLEEVE



1 Insert appropriate non-shouldered 2 Tap the abutment in the long or stealth shouldered abutment The diameter of the abutment is dictated by the anatomy of the interdental papillae. The abutment should support the papillae without encroaching upon them.



axis of the abutment post and implant well.



3 Orientate the internal flat(s) of the appropriate temporization sleeve with the external flat(s) of the abutment prior to snapping it onto the abutment.



4 Confirm the appropriateness of the temporization sleeve with a vacuum formed template. Adjust the sleeve as necessary.



5 Inject transitional crown material around the temporization sleeve.



6 Inject transitional material into the vacuum-formed template prior to re-inserting it over the temporization sleeve to form a transitional prosthesis.



7 Remove transitional prosthesis for polishing.




8 Snap the completed transitional prosthesis onto the abutment to facilitate the formation and preservation of an aesthetic soft tissue emergence profile.

OPTION TWO: TEMPORIZATION WITH A TEMPORARY OR HEALING ABUTMENT









At the time of uncovering, place a titanium temporary abutment or a plastic healing abutment. These abutments will support the soft tissue and assist in the formation of the gingival sulcus. Either abutment may be modified to achieve a desired gingival contour. Transitional crowns should not be placed on temporary or healing abutments. See Bicon catalogs for a complete listing of abutment sizes and shapes that are available.

OPTION THREE: A TRANSITIONAL PROSTHESIS IN THE AESTHETIC ZONE



5.0 x 4.5 5.0 x 6.5

1 Choose appropriately sized temporary or healing abutment. See Option #2 above.



2 Insert temporary or healing abutment into the implant well and gently seat the abutment by tapping on the head of the abutment. Removal of the abutment may be achieved with a variety of extraction forceps.



3 In aesthetic areas, a flipper may be inserted for aesthetics and function while tissue is healing around the temporary abutments



4 View of inserted provisional restoration.

IMPRESSION OPTIONS



OPTION ONE: IMPLANT LEVEL IMPRESSION



1 Choose the appropriately sized titanium impression post according to the diameter of the implant well.



2 Insert the titanium impression post into the well of the implant with finger pressure only.



3 Snap the appropriate impression sleeve onto the impression post.



2.5mn





4 Inject impression material around the plastic impression sleeve and make impression.



5 After making the impression, plastic impression sleeve should be withdrawn within the impression while titanium post remains in the implant well.



6 Remove titanium impression post from implant. Assemble the post with the appropriate implant analog. Insert this unit into the plastic sleeve in the impression. Pour soft tissue model. The laboratory technician may now choose the proper abutment for a PFM or IAC restoration.

OPTION TWO: DIRECT ABUTMENT LEVEL IMPRESSION



1 Choose an appropriately sized abutment and definitively seat the abutment with a gentle tapping force.



2 The abutment may be modified 3 Inject impression material intra-orally with irrigation or extra-orally with a #1557 carbide bur, if necessary.



around abutment for a direct impression. Pour a stone model.



4 Fabricate crown conventionally at laboratory. Insert crown with minimal cement.

OPTION THREE: INDIRECT ABUTMENT LEVEL IMPRESSION



1 Definitively seat the abutment with a gentle tapping force. Snap impression sleeves onto the unmodified abutment.



2 Inject impression material around the impression sleeves and make impression.





3 Withdraw the plastic impression sleeves in the impression. Choose appropriately sized aluminum transfer die and insert the die into the plastic sleeve.




4 Pour a soft tissue model. Fabricate crowns conventionally. See Bicon Technique Manuals for further information on this procedure.











SELECTION GUIDE








STEALTH SHOULDERED ABUTMENT




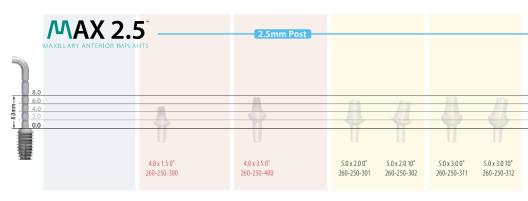



SELECTION GUIDE













WORLD HEADQUARTERS

501 Arborway

Boston, MA 02130 USA

TEL 800.88.BICON = 617.524.4443 FAX 800.28.BICON = 617.524.0096

www.bicon.com = support@bicon.com